

IC-OH and IC-OH Plus Devices

Introduction

Maxi-Clean™ and Extract-Clean™ IC Devices are solid-phase extraction devices used to eliminate matrix interferences from samples prior to analyses by ion chromatography. Each device consists of either 0.5mL or 1.5mL of polystyrene-based packing sandwiched between polyethylene frits within an injection-molded medical-grade polypropylene housing (Figure 1). Samples and wash solvents are passed through the packing using a luer hub syringe (for Maxi-Clean™) or a vacuum manifold (for Extract-Clean™). As sample comes in contact with the packing, specific chemical interactions take place which selectively retain certain components of the matrix in the device while the remaining components pass through the device outlet. The chemical characteristics of the packing dictate which sample components are retained. Seven chemistries are currently available.

Successful application of IC devices requires:

1. proper conditioning of the device prior to sample application,
2. application of the sample at a rate slow enough to allow the chemical interaction to take place while the sample is in the device, and
3. control of sample size to keep within the device's capacity.

The following information provides general recommendations for the use of IC-OH devices. This procedure may be modified to accommodate samples with different characteristics.

NOTE: The Maxi-Clean™ and Extract-Clean™ IC-OH devices are packed with polystyrene-divinylbenzene based anion exchanger in the quaternary amine functional group. The amine functional groups give this product the strong, unpleasant fishy smell. This smell is a normal part of the product and does not affect the performance of the devices.

General Information


Maxi-Clean™ and Extract-Clean™ IC-OH provide a reliable method for the adjustment of pH of acidic samples prior to the analysis of cations by ion chromatography. They may also be useful for preconcentrating anions from dilute samples prior to the analysis of anions. IC-OH devices contain either 0.5mL or 1.5mL of quaternary ammonium anion exchange resin in the hydroxide form. The hydroxide contained on the packing reacts with hydronium from the sample to form water thereby increasing pH. In this process, anions from the sample are taken up by the resin to replace the hydroxide consumed in the neutralization reaction. The net result is removal of hydronium (and an equivalent amount of sample anions) from the matrix. Hydroxide is weakly retained by the resin and is readily displaced by most other anions. Sample preconcentration is accomplished by passing a large volume of sample (with low anion concentration) through the device and eluting the retained anions in a smaller volume.

For more information on the use of Maxi-Clean™ IC cartridges and the recovery obtained with each please see:

R. Saari-Nordhaus, J.M. Anderson, Jr. and I.K. Anderson, *Am. Lab.*, August (1990) 18.

I.K. Anderson, R. Saari-Nordhaus and J.M. Anderson, Jr., *J. of Chromatography*, 546 (1991) 61-71.

Figure 1

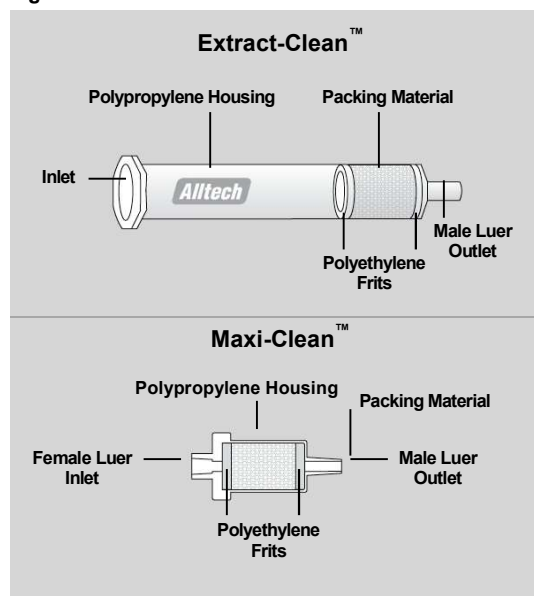

Flow Rate

The devices have a number of flow-dependent parameters that may affect results. In general, high flow rates, particularly in the sample loading step, will decrease the performance while low flow rates will improve the extraction process. Low flow rates allow the sample to diffuse into the packing thus increasing capacity and improving the efficiency. The recommended flow rate for sample loading is 1mL/minute or less.

Sample Mass

Each device contains either 0.6 or 1.5 milliequivalents of hydroxide (for the 0.5mL or 1.5mL device, respectively), which under ideal conditions will remove an equal amount of hydronium or other anions from the sample. In practice, this maximum capacity may not be realized. The nature of the sample (concentration, ionic strength, solvent) and the rate at which the sample is loaded into the device will affect the capacity. Where possible, adjust sample size to use 50% or less of the device's absolute capacity. Larger amounts of hydronium or other anions may be removed by using two or more Maxi-Clean™ cartridges in series. If the amount of hydronium or other anions in the sample is unknown, a test extraction should be performed to determine the correct sample size.

Sample Volume

The internal volumes of the different devices include the flow passages and interstitial packing volume. Although it is possible to recover all but 100µL (for the 0.5mL devices) or 150µL (for the 1.5mL devices) of sample with an air purge, best results are obtained when the sample volume greatly exceeds the internal volume of the cartridge.


| Device | Bed Size | Internal Volume |
|----------------------|----------|-----------------|
| Maxi-Clean™: | 0.5mL | 300µL |
| Maxi-Clean™ Plus: | 1.5mL | 650µL |
| Extract-Clean™: | 0.5mL | 2.5mL |
| Extract-Clean™ Plus: | 1.5mL | 1.5mL |

Example

Cations in 1M Nitric Acid

Procedure:

1. Apply 2mL of sample to a preconditioned cartridge.
2. Discard first 1mL of eluate.
3. Collect and analyze remaining eluate.

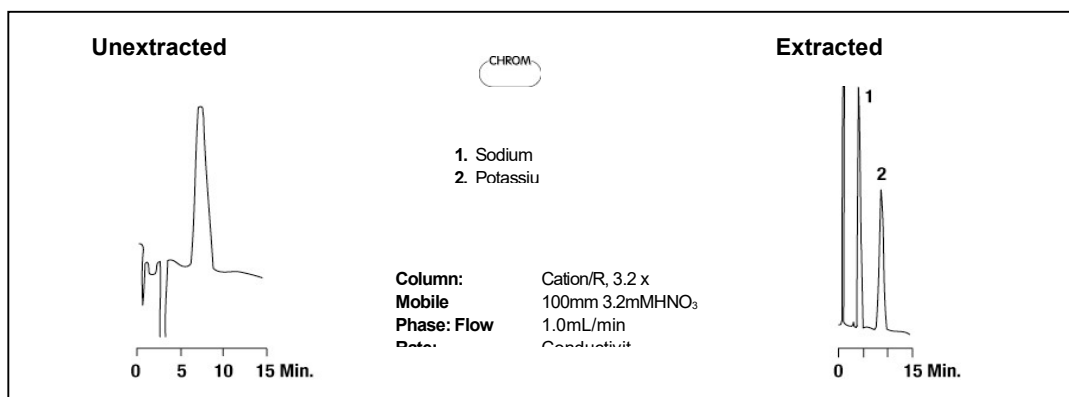

www.sstarpure.com

S*Pure Pte Ltd, Singapore

Telephone: +65 656 339 01 Fax: +65 656 339 31 E-mail: corporate@sstarpure.com

EXTRACT-CLEAN™ and MAXI-CLEAN™ are trademarks owned by S*Pure Pte. Ltd.

The information presented herein is derived from our testing and experience. It is offered for your consideration and verification. Since operating conditions vary significantly, and are not under our control, we disclaim all warranties on the results that may be obtained from the use of our products. S*Pure Pte. Ltd. cannot be held responsible for any damage or injury occurring as a result of improper installation or use of its products. S*Pure reserves the right to change prices and/or specifications without prior notification

General Procedure

1. **Precondition the Device.** Pass 5 to 10mL of IC grade water through the device. This removes interstitial contaminants and wets the packed bed. For trace analysis work, repeat the rinsing procedure until the eluant is free from interferences.
2. **Load the Sample.** Load the entire sample at 1mL/minute or less. The total amount of hydronium or other anions contained in the sample should not exceed the device capacity and preferably should be below 50% of total capacity. Discard the first 1mL of eluate. Collect the remaining eluate for analysis.
3. **For pH Adjustment.** Discard the first 1mL of eluate. Collect the remaining eluate for analysis.

Other IC Devices

| Device | Retains |
|----------------------|---|
| IC-RP: | Hydrophobic Components |
| IC-OH: | Anions (pH increase) |
| IC-H: | Cations (pH reduction) |
| IC-Ag: | Chloride, Iodide, Bromide |
| IC-Ba: | Sulfate |
| IC-Na: | Cations (no pH change) |
| IC-Chelate: | Polyvalent Metal Ions |
| IC-Mixed Mode RP-OH: | Hydrophobic Components and Anions (pH increase) |
| IC-Mixed Mode RP-H: | Hydrophobic Components and Cations (pH reduction) |

IC-OH Devices

| Description | Volume | Qty | Part No. |
|---------------------------|--------|-----|----------|
| Maxi-Clean™ IC-OH | 0.5mL | 50 | 5122573 |
| Maxi-Clean™ IC-OH Plus | 1.5mL | 25 | 5122567 |
| Extract-Clean™ IC-OH | 0.5mL | 50 | 5122909 |
| Extract-Clean™ IC-OH Plus | 1.5mL | 30 | 5122033 |

S*PURE
www.sstarpure.com